
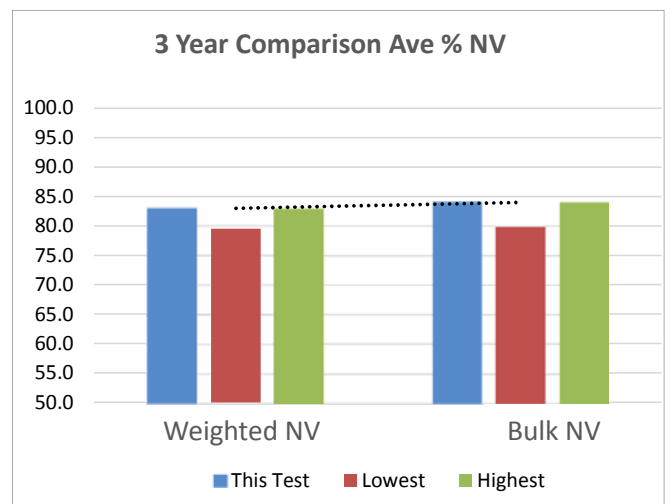


PRODUCT INFORMATION SHEET

GENERAL INFORMATION			
PIT NAME	Southgates	DATE	October 10th 2018
LOCATION	Geraldton (E)	LAB NO. LIME WA REF.	S2339 2LLS18/4426
DESCRIPTION	Limesand	SCREENED SCREEN SIZE	No
WEIGH SYSTEM	Compuload Loader Scales [Accredited weigh system verified by Trade Measurement Services]		

CODE OF PRACTICE APPROVED LABORATORY REPORT				
SIEVE RANGE (MM)	% WEIGHT		% NEUTRALISING VALUE	
	THIS TEST	3 YEAR PIT RANGE	THIS TEST	3 YEAR PIT RANGE
0.000 - 0.125	2.2	2.2 : 2.9	86.0	86.0 : 88.1
0.125 - 0.250	62.2	62.2 : 66.6	85.0	82.4 : 85.0
0.250 - 0.500	34.0	28.8 : 34.5	80.0	73.4 : 80.0
0.500 - 1.000	1.6	1.2 : 1.8	66.0	57.9 : 66.0
> 1.000	0.0	0.0 : 0.0	Insufficient Sample	0.0 : 0.0
CALCIUM (Ca) (1M HCL)	29.0	29.0 : 30.6		
MAGNESIUM (Mg) (1M HCL)	1.7	0.8 : 1.7		
SODIUM (Na) (1M HCL)	0.1	0.1 : 0.2		
WEIGHTED AVE NV			83.0	79.5 : 83.0
BULK NV			84.0	79.8 : 84.0

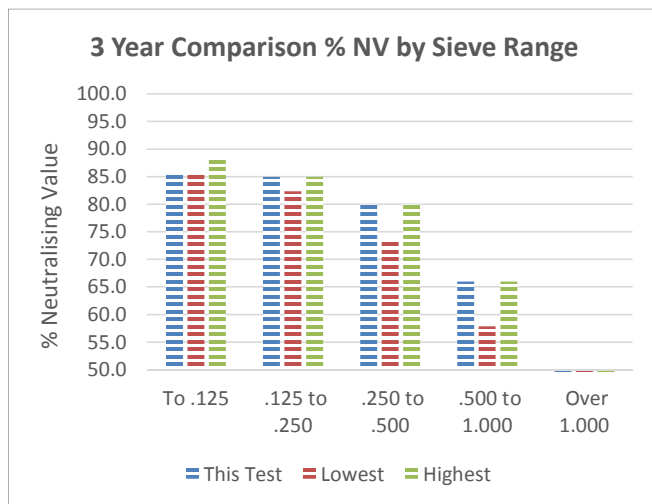

DISCLAIMER & SUPPLIER STATEMENT : The supplier states that the above analysis provided by a Lime WA Inc Agricultural Lime Industry Code of Practice approved laboratory is a true representation of the product being supplied from the nominated lime pit. Lime WA Inc requires members to provide the above details in accordance with the Code of Practice requirements but makes no claims and provides no guarantees on the quality or suitability of the product supplied. Product supplied by Lime WA Inc members occurs naturally and has a moisture retention capacity that varies according to seasonal conditions. As this cannot be controlled by suppliers, moisture level analyses are not included on this information sheet. Lime WA Inc is not responsible for any claims and/or liabilities arising from the supply and/or use of the product supplied. However, lime users are invited to contact the Association on 0419 575 737 in the event of any dissatisfaction with the product details provided by member suppliers.