

BROOMECRETE



10 Haynes Street, Broome WA 6725

T: 08 9192 1753

E: mail@broomecrete.com.au

W: www.broomecrete.com.au



LIME WA INC.

Independently Audited
Lime Suppliers



SERVING AGRICULTURE FOR 20 YEARS

Tested by a
Code of Practice
Approved Laboratory



PRODUCT INFORMATION SHEET


GENERAL INFORMATION

| | | | |
|---------------------|--------------------------------|-------------------------------|--------------------|
| PIT NAME | Broomecrete | DATE | December 23rd 2019 |
| LOCATION | Broome | LIME WA REF. LAB NO. | B1912-0241 |
| DESCRIPTION | Lime Sand | SCREENED SCREEN SIZE | Yes 5.0mm |
| WEIGH SYSTEM | Not Applicable - Loader Bucket | | |


CODE OF PRACTICE APPROVED LABORATORY REPORT

| SIEVE RANGE (MM) | % WEIGHT | | | % NEUTRALISING VALUE | |
|--------------------|-------------|--------------|------------------------|----------------------|--------------|
| | THIS TEST | NO PIT RANGE | | THIS TEST | NO PIT RANGE |
| 0.000 - 0.125 | 37.7 | 37.7 : 37.7 | | 69.2 | 69.2 : 69.2 |
| 0.125 - 0.250 | 15.7 | 15.7 : 15.7 | | 55.3 | 55.3 : 55.3 |
| 0.250 - 0.500 | 9.1 | 9.1 : 9.1 | | 60.3 | 60.3 : 60.3 |
| 0.500 - 1.000 | 7.2 | 7.2 : 7.2 | | 66.1 | 66.1 : 66.1 |
| > 1.000 | 30.3 | 30.3 : 30.3 | | 67.4 | 67.4 : 67.4 |
| CALCIUM (1M HCL) | 25.1 | 25.1 : 25.1 | | | |
| MAGNESIUM (1M HCL) | 1.2 | 1.2 : 1.2 | | | |
| SODIUM (1M HCL) | 1.1 | 1.1 : 1.1 | | | |
| | | | WEIGHTED AVE NV | 65.4 | 65.4 : 65.4 |
| | | | BULK NV | 66.1 | 66.1 : 66.1 |

3 Year Comparison % NV by Sieve Range

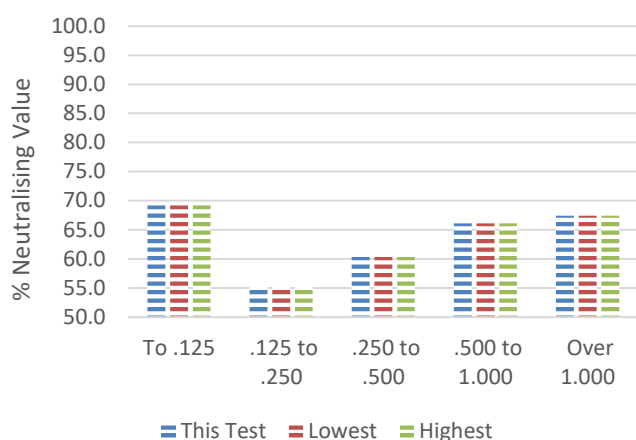

3 Year Comparison Ave % NV

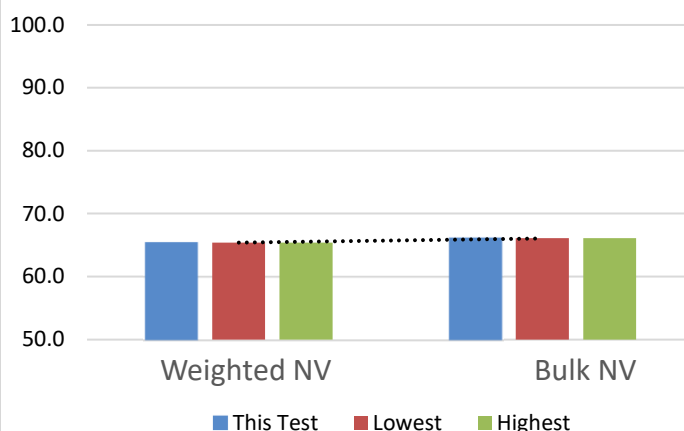

DISCLAIMER & SUPPLIER STATEMENT : The supplier states that the above analysis, provided by a Lime WA Inc Agricultural Lime Industry Code of Practice approved laboratory, is a true representation of the product being supplied. However, this test is for one lime sample collected on one day. The pit ranges show results obtained within the past three years, but please contact your supplier for analyses over a longer timeframe. Lime WA Inc requires members to provide the above details in accordance with the Code of Practice requirements, but makes no claims and provides no guarantees on the quality or suitability of the product supplied. Product supplied by members occurs naturally and has a moisture retention capacity that varies according to seasonal conditions. As this cannot be controlled by suppliers, moisture levels are not stated. Lime WA Inc is not responsible for any claims and/or liabilities arising from the supply and/or use of these products. However, lime users are invited to contact the Association on 0419 575 737 in the event of any dissatisfaction with the product details provided by suppliers.