



TEL: 1800 889 493



**LIME WA INC.**  
Independently Audited  
Lime Suppliers

**SERVING AGRICULTURE FOR 20 YEARS**

*Tested by a  
Code of Practice  
Approved Laboratory*



## PRODUCT INFORMATION SHEET


### GENERAL INFORMATION

|                     |   |                               |                   |            |
|---------------------|---|-------------------------------|-------------------|------------|
| <b>PIT NAME</b>     | Lake Preston Lime   | <b>DATE</b>                   | December 9th 2019 |            |
| <b>LOCATION</b>     | Myalup  | <b>LIME WA REF.   LAB NO.</b> |                   | B1912-0068 |
| <b>DESCRIPTION</b>  | Limestone   | <b>SCREENED   SCREEN SIZE</b> | Yes               | 2.0mm      |
| <b>WEIGH SYSTEM</b> | 100 T Weighbridge [Weigh system verified by National Measurement Institute licensed technician] |                               |                   |            |


### CODE OF PRACTICE APPROVED LABORATORY REPORT

| SIEVE RANGE (MM)   | % WEIGHT    |                  |                        | % NEUTRALISING VALUE |                  |
|--------------------|-------------|------------------|------------------------|----------------------|------------------|
|                    | THIS TEST   | 2 YEAR PIT RANGE |                        | THIS TEST            | 2 YEAR PIT RANGE |
| 0.000 - 0.125      | <b>2.7</b>  | 2.7 : 6.7        |                        | <b>75.2</b>          | 75.2 : 81.3      |
| 0.125 - 0.250      | <b>25.4</b> | 25.4 : 32.5      |                        | <b>76.5</b>          | 67.6 : 76.5      |
| 0.250 - 0.500      | <b>46.3</b> | 27.5 : 46.3      |                        | <b>76.7</b>          | 70.2 : 76.7      |
| 0.500 - 1.000      | <b>16.0</b> | 16.0 : 18.4      |                        | <b>74.0</b>          | 72.4 : 74.0      |
| > 1.000            | <b>9.6</b>  | 9.6 : 14.8       |                        | <b>85.5</b>          | 81.2 : 85.5      |
| CALCIUM (1M HCL)   | <b>29.9</b> | 27.9 : 29.9      |                        |                      |                  |
| MAGNESIUM (1M HCL) | <b>0.6</b>  | 0.5 : 0.6        |                        |                      |                  |
| SODIUM (1M HCL)    | <b>0.2</b>  | 0.1 : 0.2        |                        |                      |                  |
|                    |             |                  | <b>WEIGHTED AVE NV</b> | <b>77.0</b>          | 72.1 : 77.0      |
|                    |             |                  | <b>BULK NV</b>         | <b>78.3</b>          | 75.4 : 78.3      |

**3 Year Comparison % NV by Sieve Range**

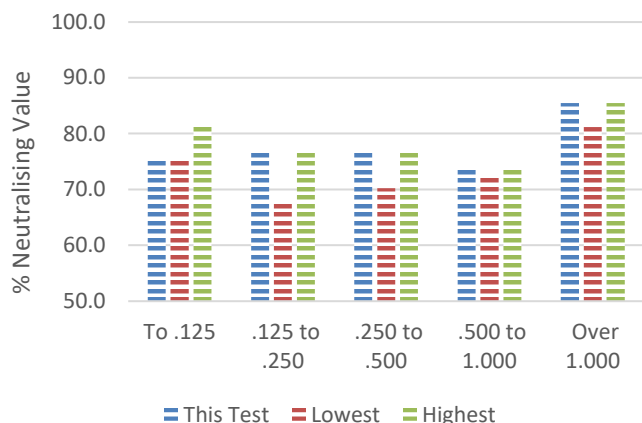

**3 Year Comparison Ave % NV**

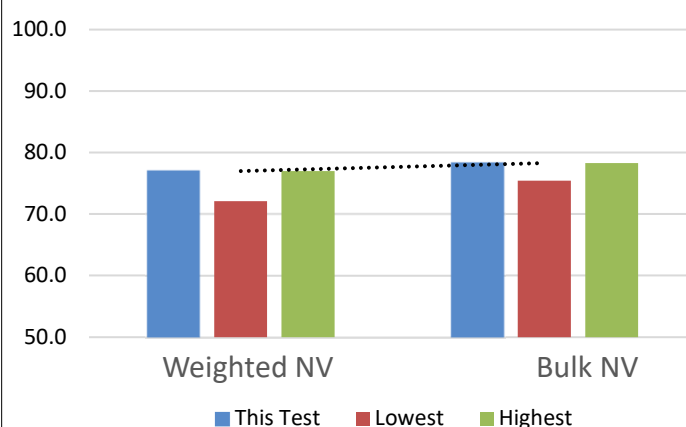

**DISCLAIMER & SUPPLIER STATEMENT :** Although the supplier states that the above analysis, provided by a Lime WA Inc Agricultural Lime Industry Code of Practice approved laboratory, is a true representation of the product being supplied, the test results are for a single lime sample collected on one day. The pit ranges show results obtained within the past three years, but analyses over a longer timeframe are available on request. Lime WA Inc requires members to provide the above details in accordance with the Code of Practice requirements, but makes no claims and provides no guarantees on the quality or suitability of the product supplied. Product supplied by members occurs naturally and has a moisture retention capacity that varies according to seasonal conditions. As this cannot be controlled by suppliers, moisture levels are not stated. Lime WA Inc is not responsible for any claims and/or liabilities arising from the supply and/or use of these products. However, lime users are invited to contact the Association on 0419 575 737 in the event of any concerns with the product details provided.