

BROOMECRETE



10 Haynes Street, Broome WA 6725

T: 08 9192 1753

E: mail@broomecrete.com.au

W: www.broomecrete.com.au



LIME WA INC.

Independently audited
by DPIRD



SERVING AGRICULTURE FOR OVER 20 YEARS



Tested by a
Code of Practice
Approved Laboratory




PRODUCT INFORMATION SHEET

GENERAL INFORMATION			
PIT NAME	Broomecrete	DATE	May 24th 2023
LOCATION	Broome	LIME WA REF. LAB NO.	LWA 23-12 B2305-0284-1256
DESCRIPTION	Lime Sand	SCREENED SCREEN SIZE	Yes 5.0mm
WEIGH SYSTEM	Not Applicable - Loader Bucket		

CODE OF PRACTICE APPROVED LABORATORY REPORT				
SIEVE RANGE (MM)	% WEIGHT		% NEUTRALISING VALUE	
	THIS TEST	3 YEAR PIT RANGE	THIS TEST	3 YEAR PIT RANGE
0.000 - 0.125	12.8	10.8 : 22.7	69.3	67.6 : 69.3
0.125 - 0.250	8.8	8.8 : 16.2	53.8	30.4 : 53.8
0.250 - 0.500	8.1	8.1 : 11.1	60.6	42.0 : 60.6
0.500 - 1.000	14.3	8.4 : 14.3	66.1	56.0 : 63.5
> 1.000	56.0	40.6 : 59.3	68.5	58.0 : 68.5
CALCIUM (1M HCL)	26.4	20.6 : 26.4		
MAGNESIUM (1M HCL)	0.4	0.4 : 1.2		
SODIUM (1M HCL)	0.4	0.3 : 0.4		
			WEIGHTED AVE NV	66.3 54.3 : 66.3
			BULK NV	66.4 54.8 : 66.4

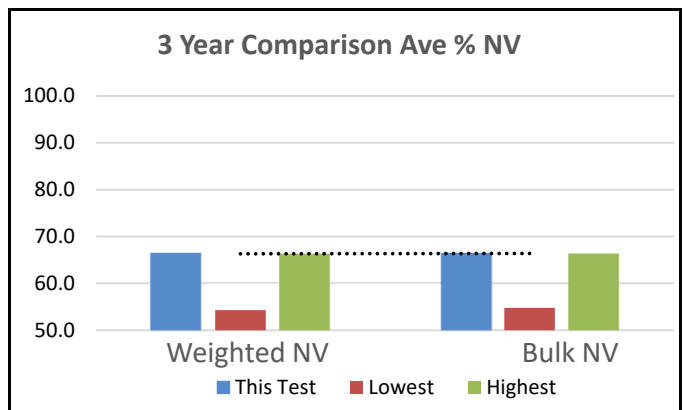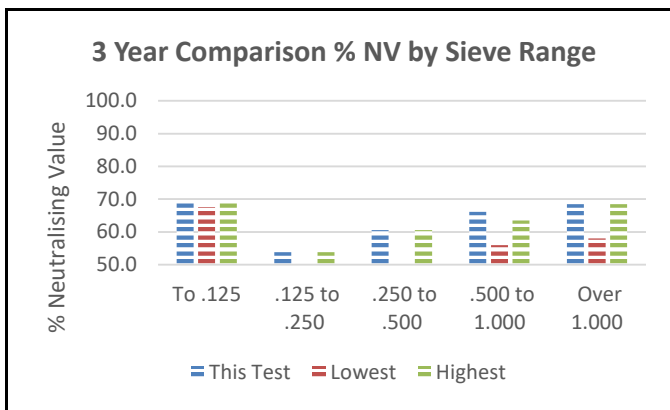



Department of Primary Industries and Regional Development

This product sample was collected by the Department of Primary Industries and Regional Development, and was submitted directly to an approved laboratory for testing as part of the Lime WA Inc. independent audit program.

DISCLAIMER & SUPPLIER STATEMENT : Although the above analysis, provided by a Lime WA Inc Agricultural Lime Industry Code of Practice approved laboratory, is a true representation of the product being supplied, the test results are for a single lime sample collected on one day. The pit ranges show audit results obtained within the past three years, but analyses over a longer timeframe are available on request. Lime WA Inc makes no claims and provides no guarantees on the quality or suitability of the product supplied. Product supplied by members occurs naturally and has a moisture retention capacity that varies according to seasonal conditions. As this cannot be controlled by suppliers, moisture levels are not stated. Lime WA Inc is not responsible for any claims and/or liabilities arising from the supply and/or use of these products. However, lime users are invited to contact the Association on 0419 575 737 in the event of any concerns with the product details.